CoMax

COMPOSITE DISPENSER

INSTRUCTIONS FOR USE

OPERATION AND FIRST TIME USE

The CoMax Composite Dispenser is intended for use with most standard composite compules. Insert the compule by pulling back on the front flange. (See Fig.1on reverse side)

Release the flange to keep compule in place. Place 4 fingers on trigger and pull back to express composite. (See Fig.2 on reverse side)

To remove compule, pull back on flange and compule will drop out by itself. (No need to touch compule, see Fig. 3 on reverse side)

Safety Precautions

Before expressing composite, always ensure that the compule is fully seated in the barrel and secured with the spring loaded collar.

Always ensure that your brand and style of compule is compatible with the CoMax. Test compatibility by expressing material onto a pad or tabletop prior to patient use.

Cleaning and Sterilization

NON STERILE

The CoMax Composite Dispenser may be autoclaved in a steam autoclave. It is not recommended that it be chemclaved. It may also be wiped down with a disinfectant such as CaviCide®, Envirocide® or Cidex®.
DO NOT SOAK THE COMAX DISPENSER IN DISINFECTANT SOLUTION.

WARRANTY

The CoMax Composite Dispenser has a warranty for a period of 2 years. For a no cost extended warranty register at www.addent.com.

REPLACEMENT PARTS

There are no replacement parts.
PN 120000 CoMax Composite Dispenser

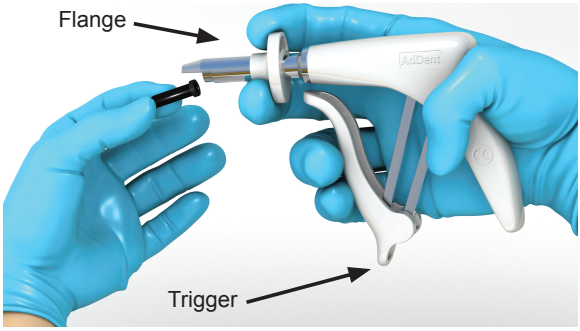

Figure 1

Loading the compule into the CoMax dispenser

Figure 2

Holding the CoMax to express composite

Figure 3

Removing the used compule from the CoMax dispenser

MANUFACTURER

AdDent, Inc.
43 Miry Brook Road, Danbury CT 06810
Phone: 203-778-0200, Fax: 203-792-2275
Email: info@addent.com
Website: www.addent.com

CE

EC REP

EMERGO EUROPE
Molenstraat 15
2513 BH, The Hague
The Netherlands

QAS INTERNATIONAL
ISO 9001:2008
REGISTERED FIRM

ISO CERTIFIED

P/N 660104 REV D 5/2017