MICROLUX • *Mini*

AdDent Incorporated

Available Accessories

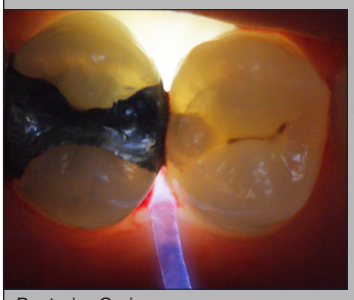

Posterior Caries

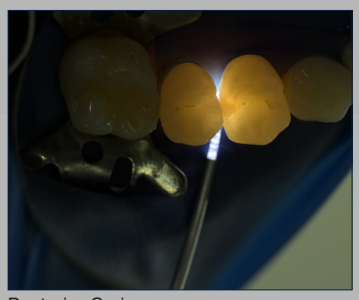

Posterior Caries

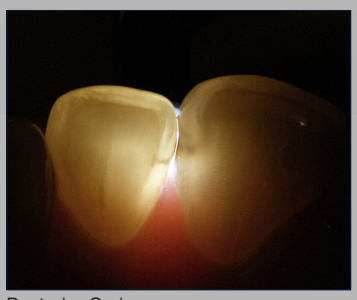

Posterior Caries

Cracks

43 Miry Brook Road • Danbury, CT 06810 • (203) 778-0200

AdDent INCORPORATED *Advancing Dental Excellence*

ISO 9001 CERTIFIED & 13485 COMPLIANT | ALL PRODUCTS ARE FDA CLEARED

Made in the USA | www.addent.com

THE MICROLUX MINI

The Microlux Mini puts the power of transillumination in the hands of dentists in places where cost is of major concern. It operates with 2 standard AAA batteries, universally available. It's used to visualize caries, cracks, and calculus without X-rays. It accepts the complete range of Microlux accessories which include 2- and 3-mm glass lightguides, Endo lite, .75 mm proximal light guide and lighted mirrors. All accessories are autoclavable.

FEATURES

- Autoclavable Light Giude
- Accepts All Microlux Plug-in Accessories
- Uses Widely Available AAA Batteries

BENEFITS

- Easy Handling
- Better Visualization of Caries, Calculus and Cracks
- Easy One Finger Operation

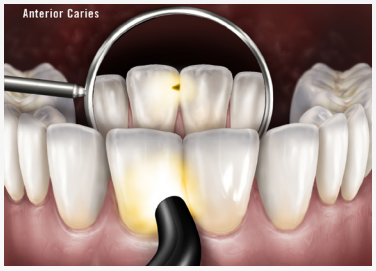

Anterior Caries: Anterior caries can be visualized by placing the probe on the labio-cervical region of the tooth and examine from the lingual. **Shown above: 3mm P/N 630003, 2mm P/N 600045, Pedo P/N 110066.**

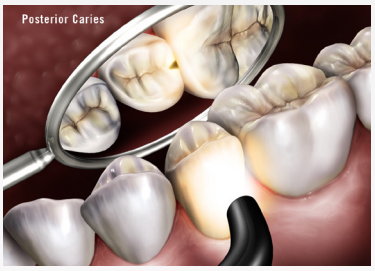

Posterior Caries: To visualize posterior proximal decay, place the probe on the cervical area of the tooth. Caries appear as a dark shadow on the occlusal surface. **Shown above: 3mm P/N 630003, 2mm P/N 600045, Pedo P/N 110066.**

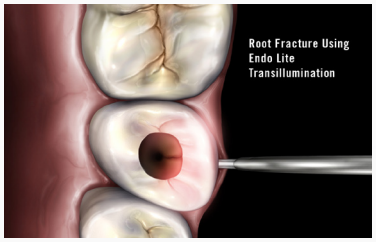

Root Fracture: Root fractures can often be detected by using the Endo Fiber tip. Place it either buccally or lingually in the gingival sulcus. A fracture line will appear dark via transillumination from the outside to the inside of the canal. **Shown above: Endo-Light Guide P/N 640035.**

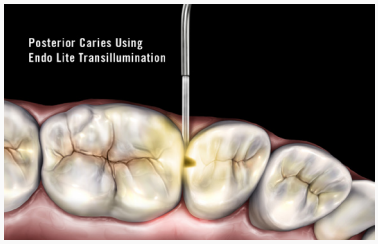

Posterior Caries: Caries can be detected using the Proximal Caries fiber tip. Place the lighted fiber tip interproximally under the marginal ridge. View from the occlusal. This method often shows caries with high definition. **Shown above: Proximal Caries P/N 640072.**

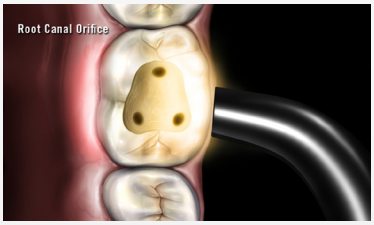

Root Canal Orifice: To help locate root canal orifice, place the light source on the buccal or lingual cervical region of the tooth. **Shown above: 3mm P/N 630003, 2mm P/N 600045, Pedo P/N 110066.**

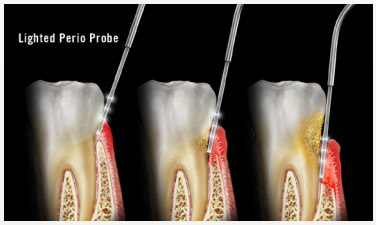

Periodontial Disease: To detect the depth of the periodontal pockets and gingival recession, use the lighted Perio Probe and insert the tip in the gingival sulcus. The depth indications are 3, 5, and 7mm. **Shown above: Perio Probe P/N 640041.**

MD EC REP EMERGO EUROPE Westervoortsedijk 60, 6827 AT Arnhem The Netherlands CE ISO 13485 COMPLIANT

Follow us on social media: info@addent.com

SCAN ME

AdDent INCORPORATED *Advancing Dental Excellence*

ISO 9001 CERTIFIED & 13485 COMPLIANT | ALL PRODUCTS ARE FDA CLEARED

Made in the USA | www.addent.com