Microlux transilluminator with the new interproximal tip that slides under the proximal contact

From ADDENT

Dentistry by Dr. Howard Strassler

Microlux with transillumination tip for interproximal diagnosis

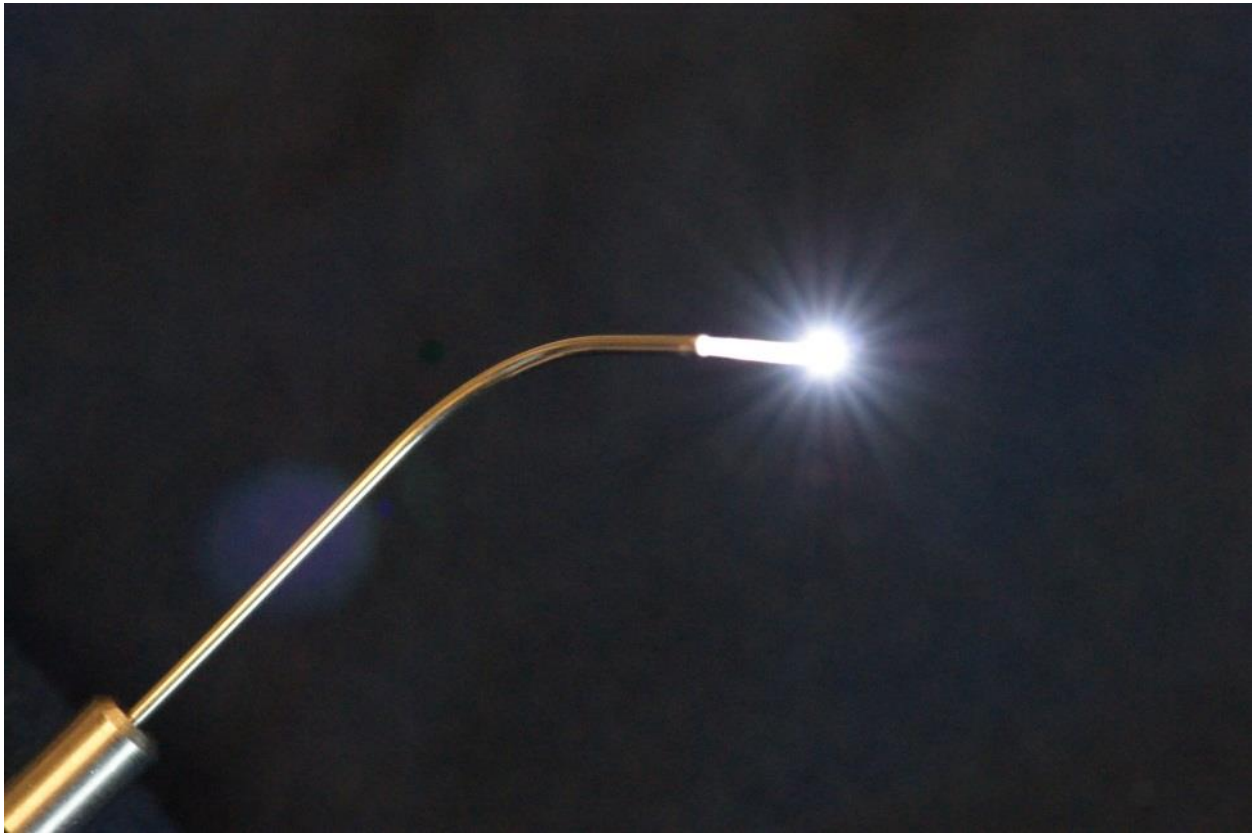

Tip should be positioned just at the interproximal

Too far through the interproximal

Correct placement of tip.

Interproximal caries #12-D (#13-MOD has been restored with amalgam)

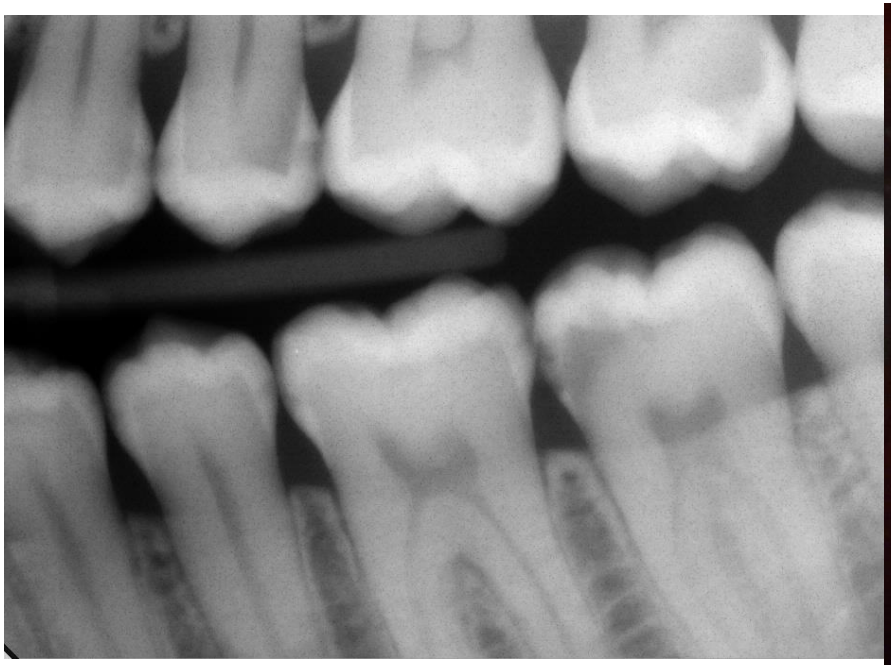

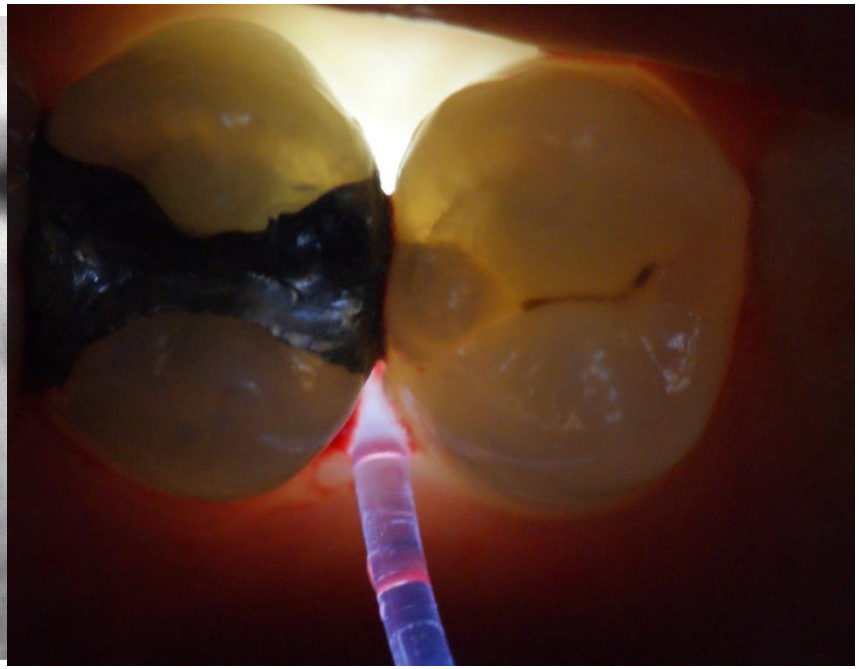

Transilluminated with the new interproximal tip that slides under the contact

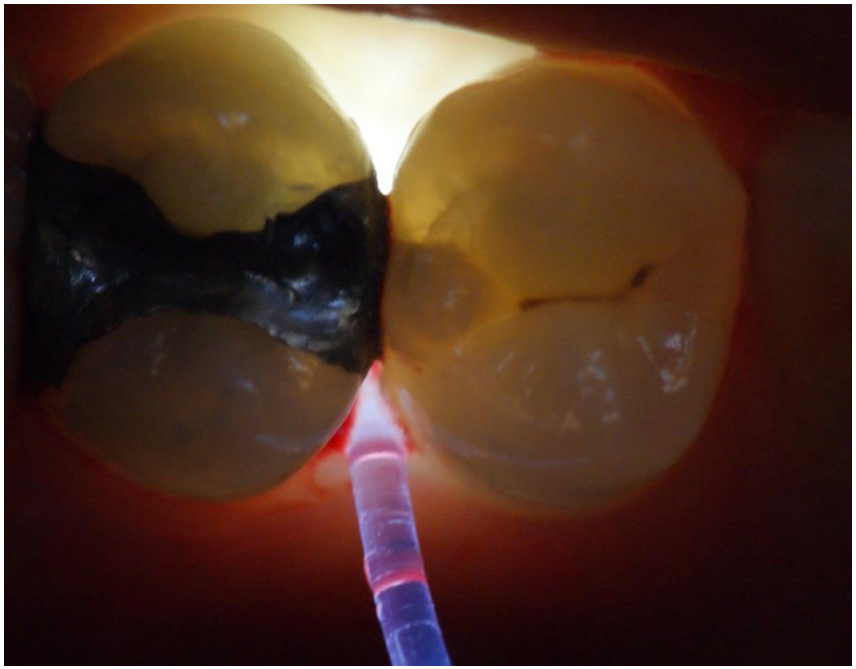

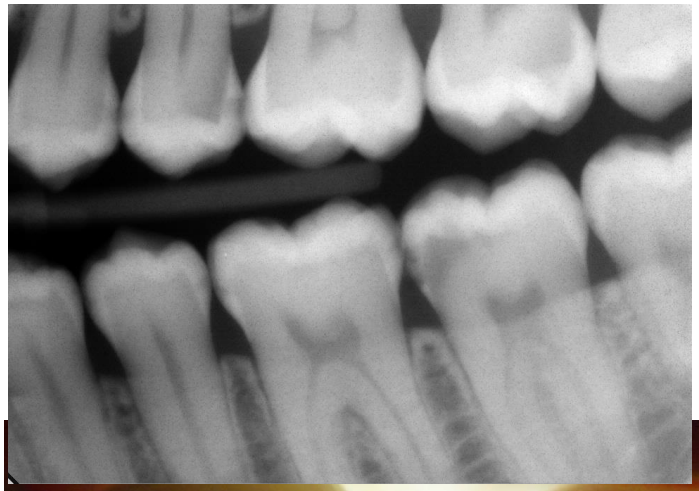

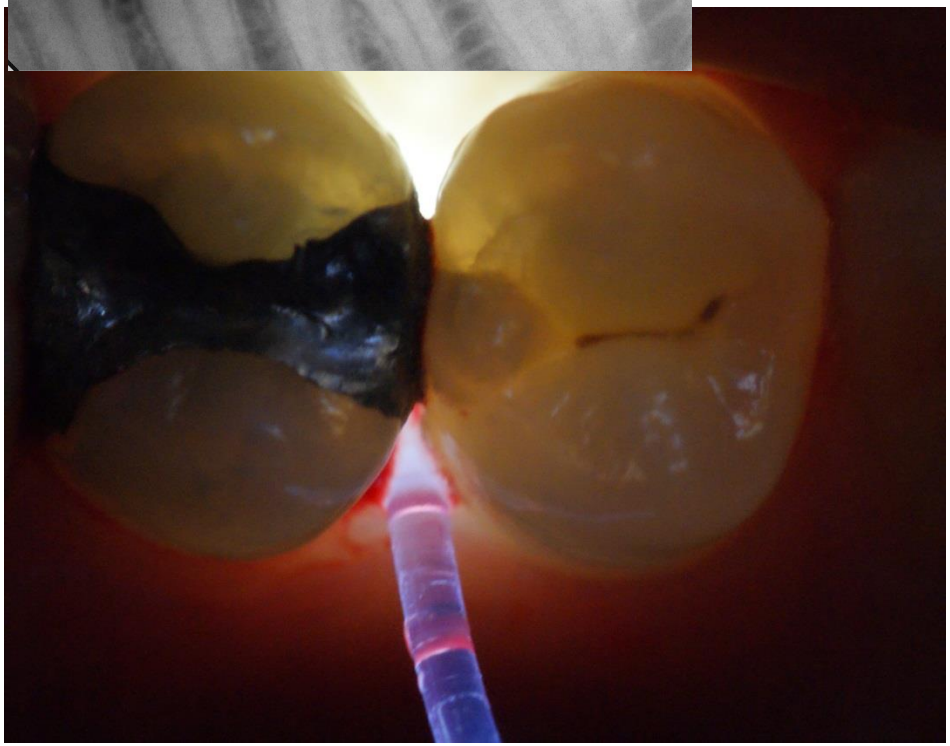

final preparation
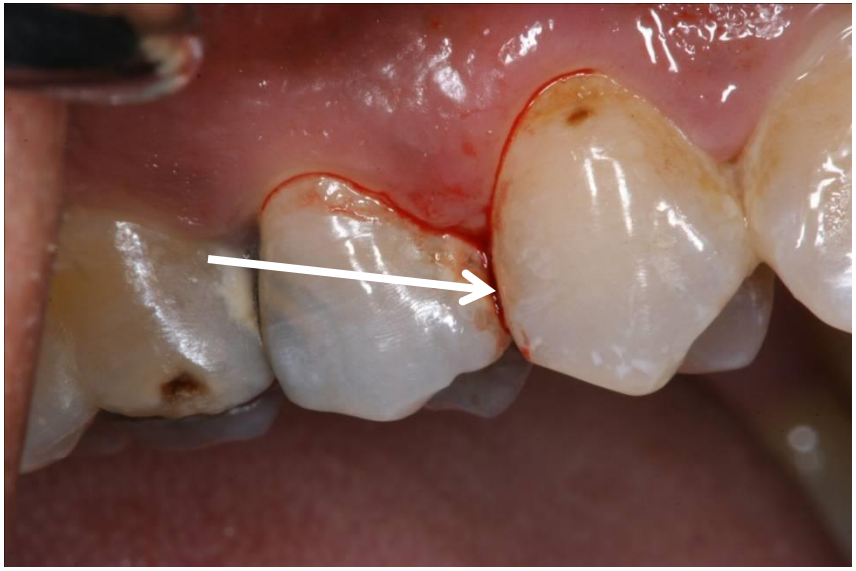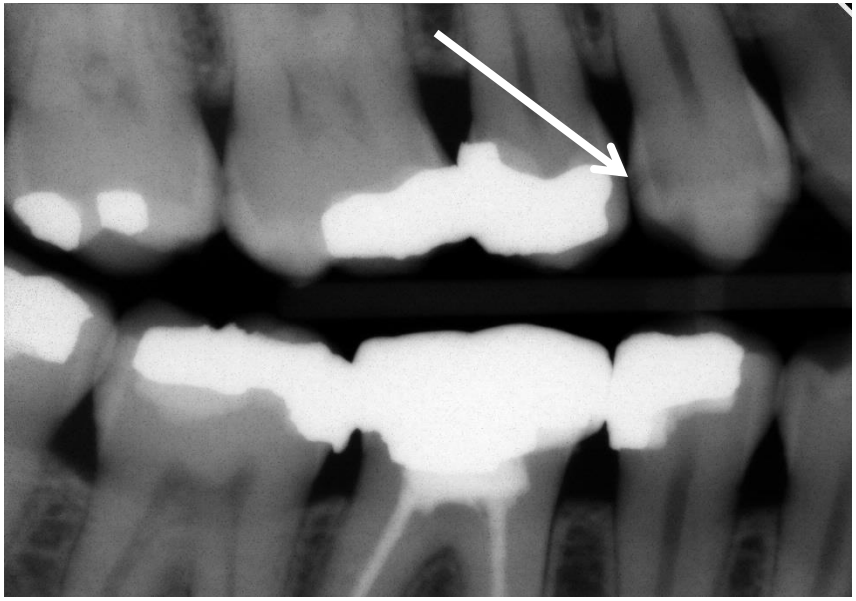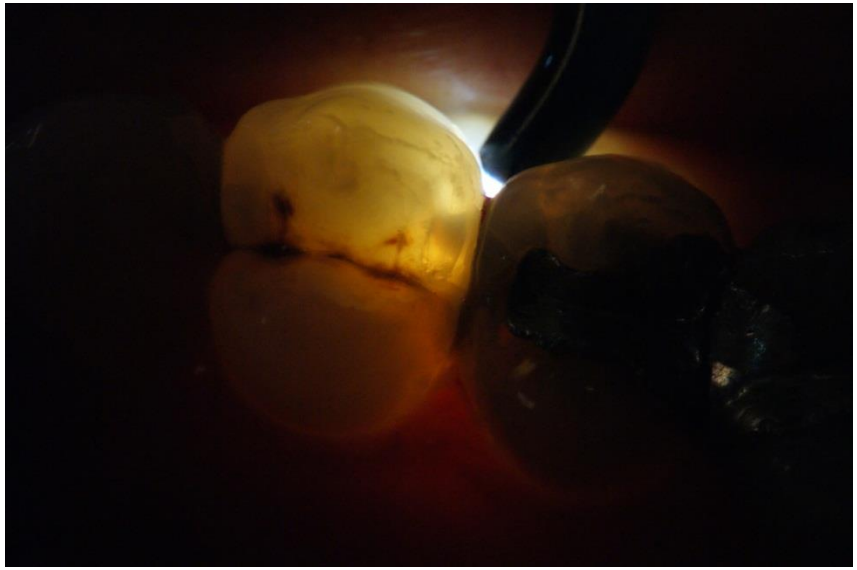
Posterior 2 mm tip